



**Significant Events:** May 26<sup>th</sup> 2017 to June 22<sup>th</sup> 2017


- **5/26 RTMQC:** Changed all Filters.
- **6/14 RTMQC:** Changed all Filters.

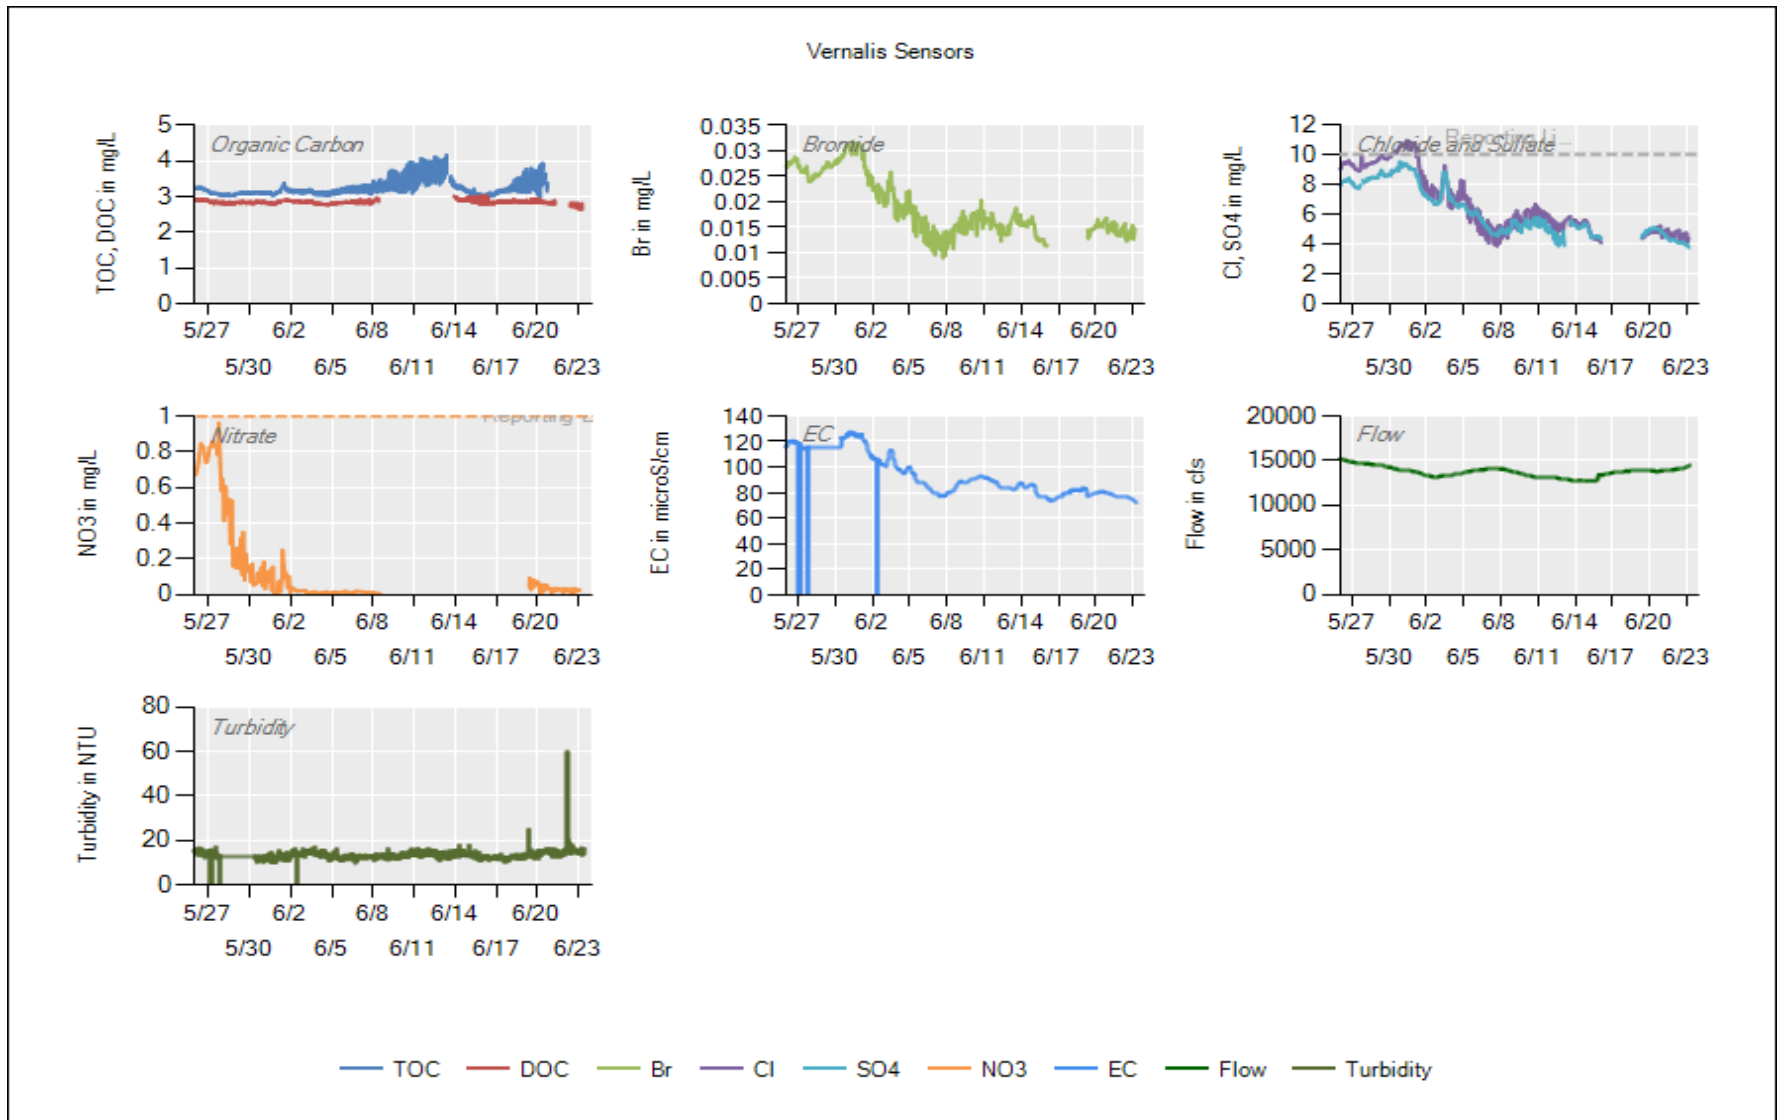


**Events:** 6/1 = Filter and housing rinse. 6/13 = QC and all filters changed. Debris removed from front of station. Pump intake cleaned. IOS/sampling manifold for carbon analyzer cleaned. **Note:** Still having problem with valves for sampling manifold on the Sievers carbon analyzer. Site visit planned for afternoon of Friday 6/23 (after this graphical update was produced).

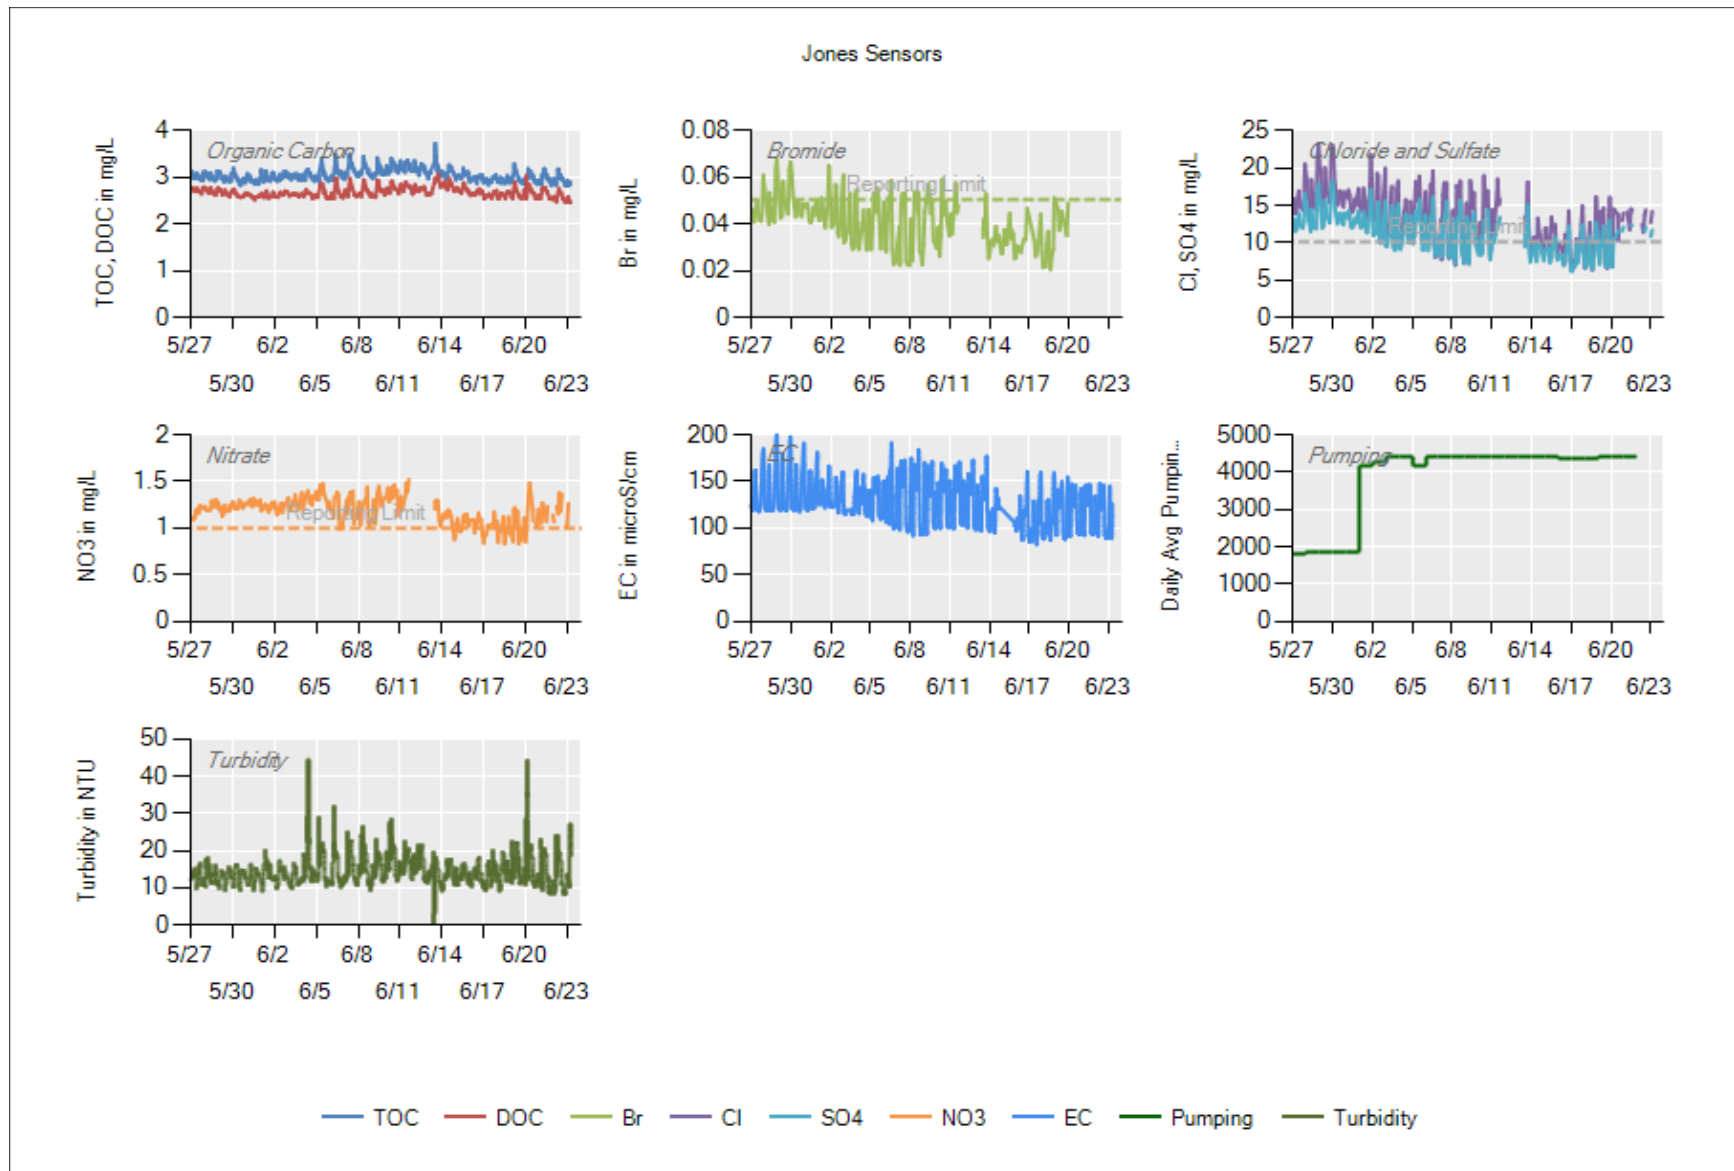

6/13 – Changed the 100 and 0.45 um filters. Organic carbon QC samples did not pass.

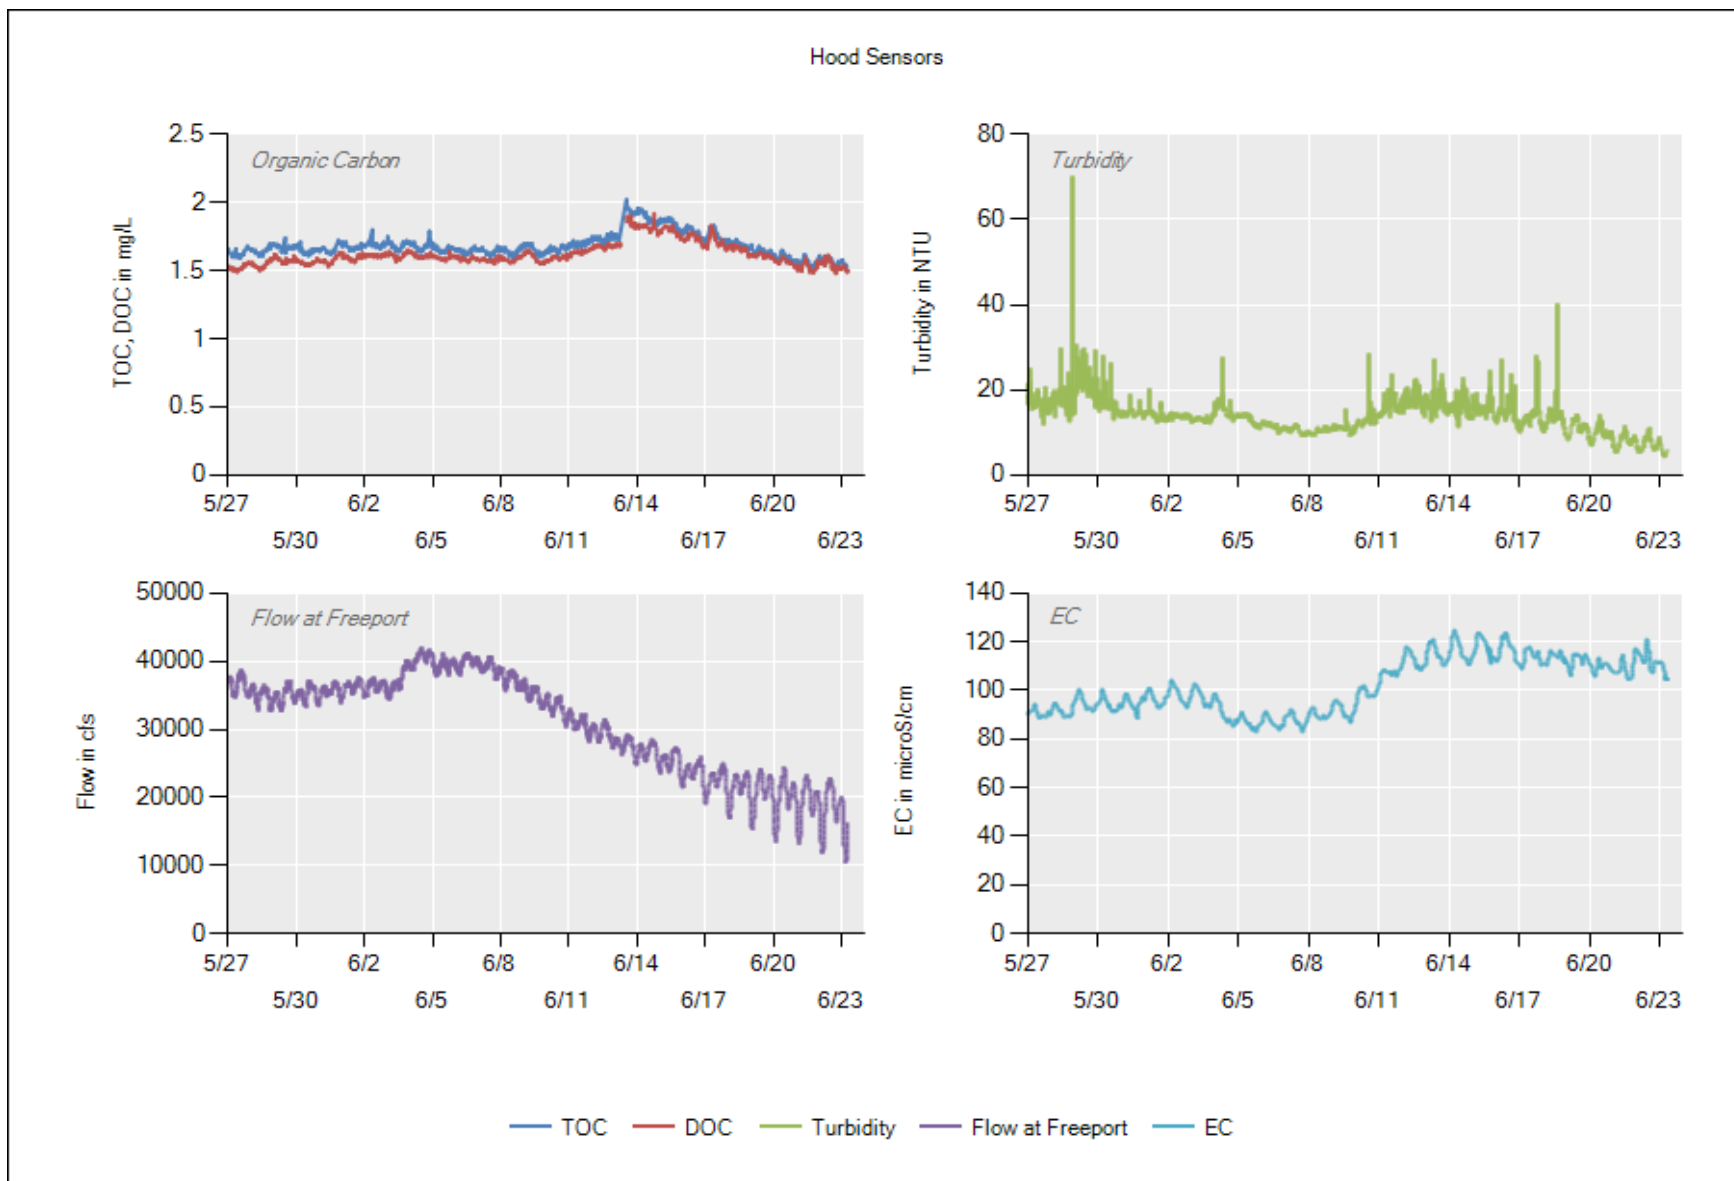

6/13 – Changed the 1 um and 0.45 um filters, cleaned the 50 um filter, analyzed all QC samples.

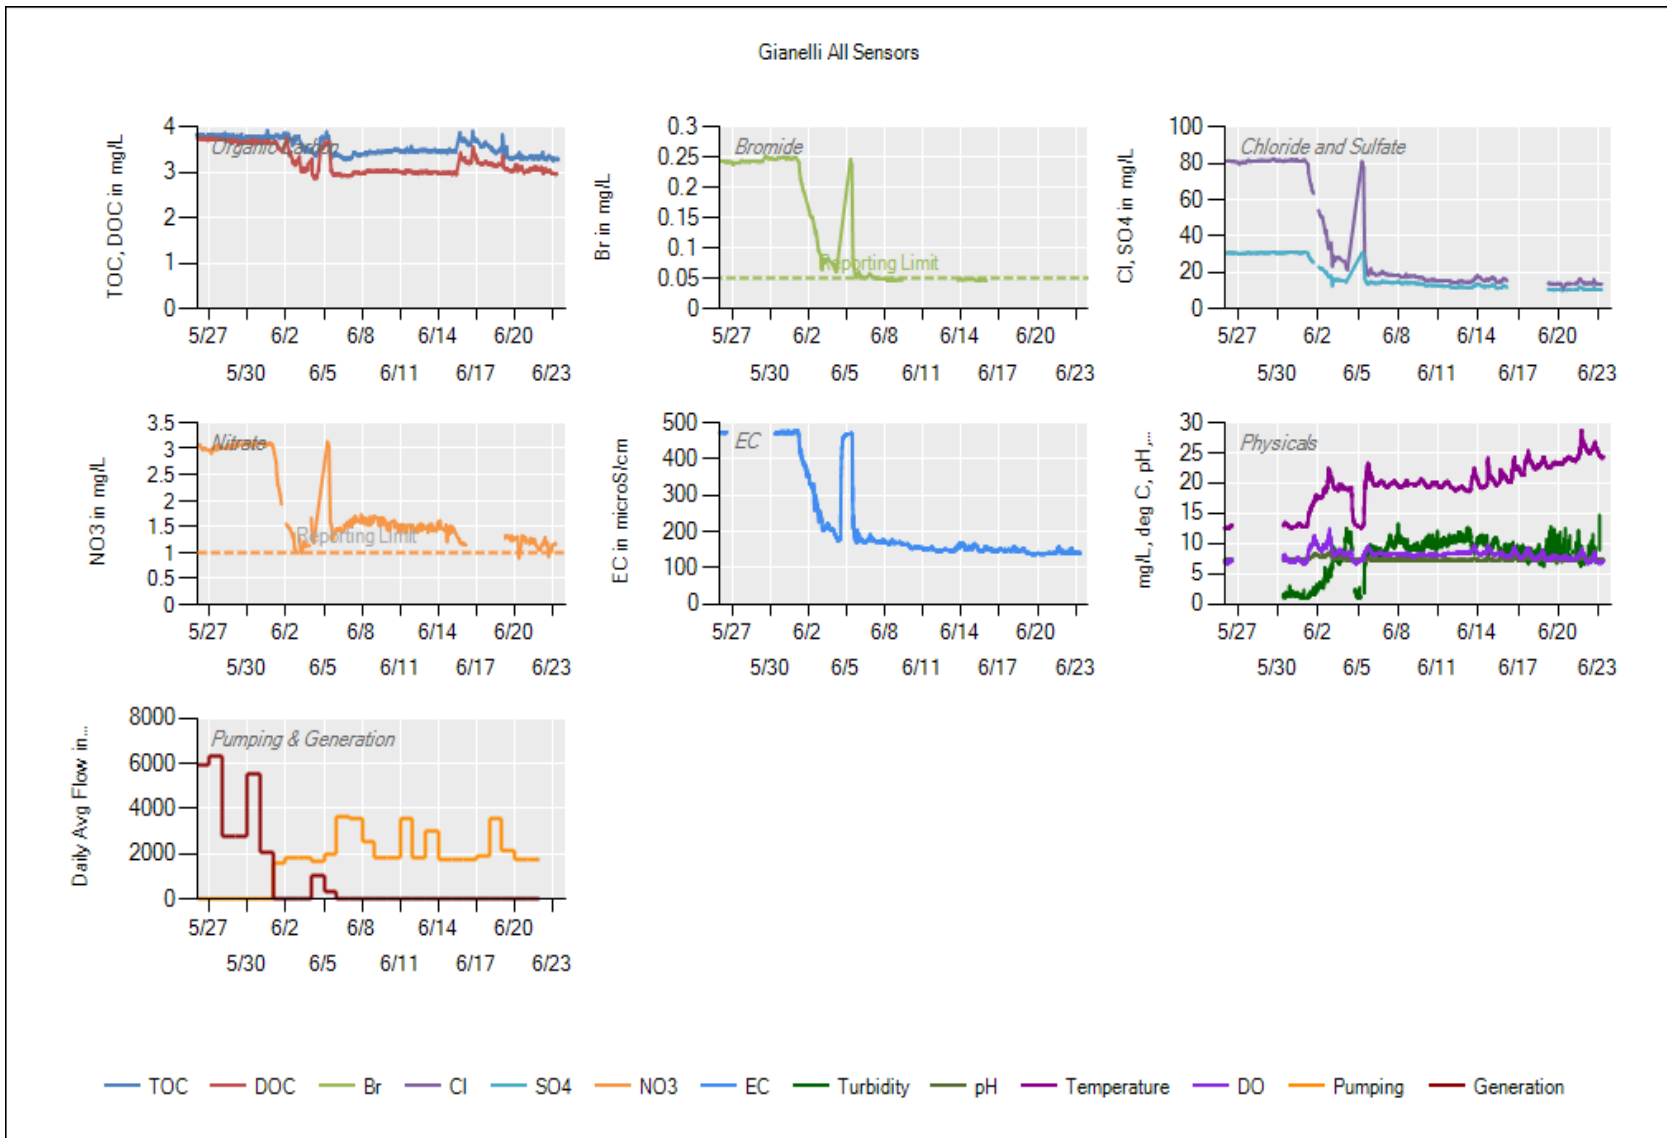

- The YSI was not set to log over the weekend of 5/26.
- The anion analyzer shutdown on 6/4 and was restarted on 6/5 during a brief period of generation.
- The anion analyzer again shutdown on 6/16 and was not restarted until the next Monday.

